

Framework Modules for Electromagnetic Sensors

Nikola Draganov¹ and Lyubomir Spasov²

¹Faculty of Electrical Engineering and Electronics at Technical University of Gabrovo
4 Hadji Dimitar Str.,
Gabrovo 5300, Bulgaria
ndrag@abv.bg



²Faculty Electrical Engineering and Electronics at Technical University of Gabrovo
4 Hadji Dimitar Str.,
Gabrovo 5300, Bulgaria

ABSTRACT: *Sensors with magnetic fields have more comprehensive applications in industries and homes. The electric power measurement with a magnetic field can measure electrical parameters that use sensors. In this work, we have created a sensor framework for measuring electrical current. We have designed an experimental module with a magnetosensitive circuit with the necessary elements. We have further explained the block diagram with general electric circuits and results.*

Keywords: Galvanomagnetic Sensors, Current Sensors, Electromagnetic Sensors, Hall Sensors, Electric Current Measurement

Received: 2 December 2022, Revised 5 March 2023, Accepted 16 March 2023

DOI: 10.6025/jet/2023/14/2/45-50

Copyright: with Authors

1. Introduction

With the development of newer electronics technologies, in particular, sensor technology – Hall effect sensors are becoming increasingly popular in engineering environments as the primary means of measuring electrical current with high reliability, performance, sensitivity and accuracy. They are successfully applied for measurement and control of the parameters of electrical circuits. Today, Hall's components are widely used in almost all measuring device and household appliances in light and heavy industries

Interest for sensors technologies is the contactless measurement of the parameters of electrical signals and more precisely, of the electrical parameters of power circuits. This method has many advantages the most important among them is the galvanic

separation of the two circuits – the measured and measuring [1-10].

There are various sensor transducers that allow contactless measurement of circuitry parameters. They work on different physical principles – optical, inductive, magnetic, galvanomagnetic. The last are widespread in modern electronics and automation. They have some very important advantages over others, namely easy signal processing, repeatability, high sensitivity to broadband frequency signals, reliability, and more [1-6].

The purpose of the present study is to design, develop and study a real-time sensor module for electrical current measurement based on a modern magnetosensitive integrated circuit with a Hall element.

2. Presentation

The block diagram of the realized module is shown in Figure 1.

The main unit is the magnetosensitive integrated circuit (MIC), which converts the magnetic field into an electrical signal, a voltage stabilizer (VS) providing the required DC mode and an interface circuit (IC) that forms the signal in a suitable form for follow processing.

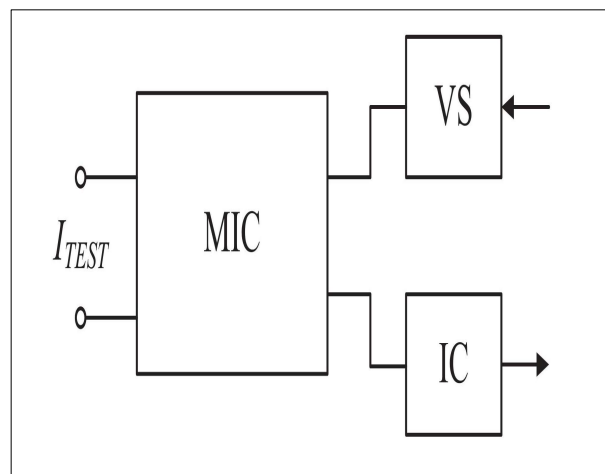


Figure 1. Block diagram of the measuring module

The developed model is a single-PCB module with detached terminals, connecting the measured circuit to the current terminals of the magneto-sensitive IC. The last is a monolithic silicon chip with a magnetosensitive element and a processing circuit mounted on a current-carrying bus the ends of which are the IP + and IP- current measuring terminals of the integrated circuit. When a current flows through the bus, a magnetic field is formed around it which is detected by the sensor integrated in the package, and it converts the magnetic field into a proportional output voltage.

Figure 2 shows the circuit diagram of the developed module.

The stabilizer block is built with an integral voltage stabilizer of type LM7805 (IC1). The developed device is of an experimental type. The supply current I_S that is required for it does not exceed 50mA. Of course, when installing the device into portable measurement and battery-powered systems, it is necessary to replace it with an appropriate low dropout voltage regulator.

The magnetosensitive integrated circuit (IC2) of type ACS710 for electrical measurement with Hall element is produced by Allegro Micro Systems Company [9]. It provides a precise solution to convert the size of alternating and direct current in output voltage. Due to its small dimensions, it can be embedded in the package of most electronic devices for electrical currents measurement in current protections, instantaneous values of electrical signals, control and diagnostics of power transducers and electrical equipment.

In this type of IC, the current terminals (IP + and IP-) must be connected to the measured current loop in a given circuit. Current terminals IP+ and IP- of the integrated circuit have respectively four physical terminals internally integrated into a common copper conductor with $R_{IP+IP-}=1m\Omega$?. They provide the carrying out and measurement of electrical current up to 25A. The sensor signal processing scheme allows to measure positive and negative values of electrical current, but it is necessary to observe the polarity of the IP+ and IP- terminals when entering the circuit. The selected magnetosensitive integrated circuit is equipped with Fault and Fault_EN functions. It can provide additional feedback to detect the maximum value of the measured current. This improves the functionality and reliability of the sensor device. The speed of the sensor can be set by selecting a suitable CF capacitor.

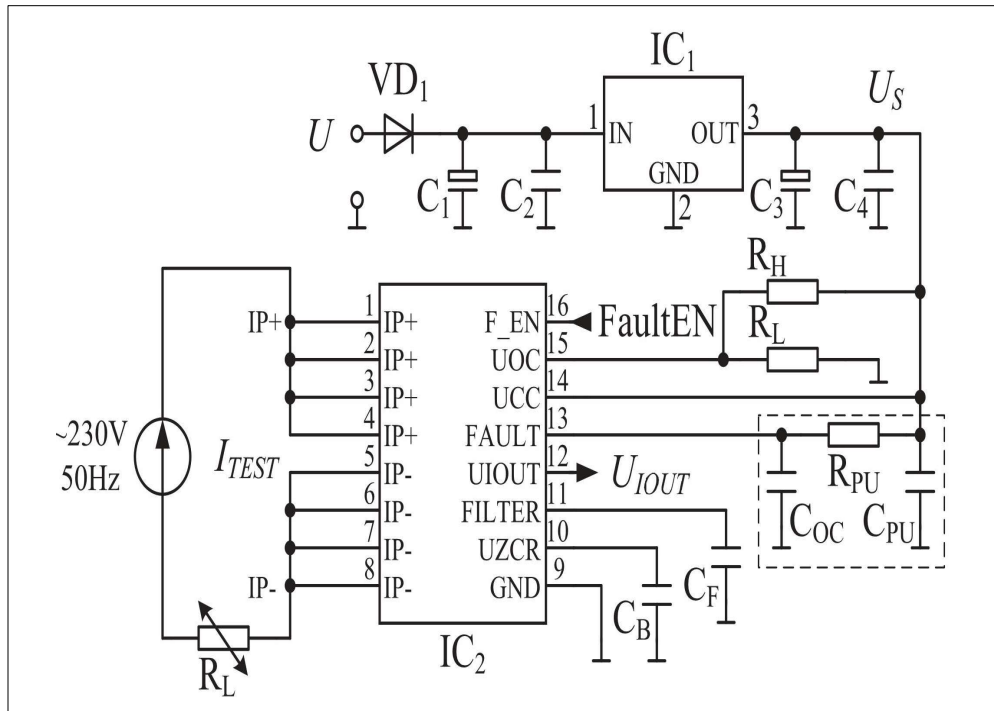


Figure 2. The circuit diagram of the developed module

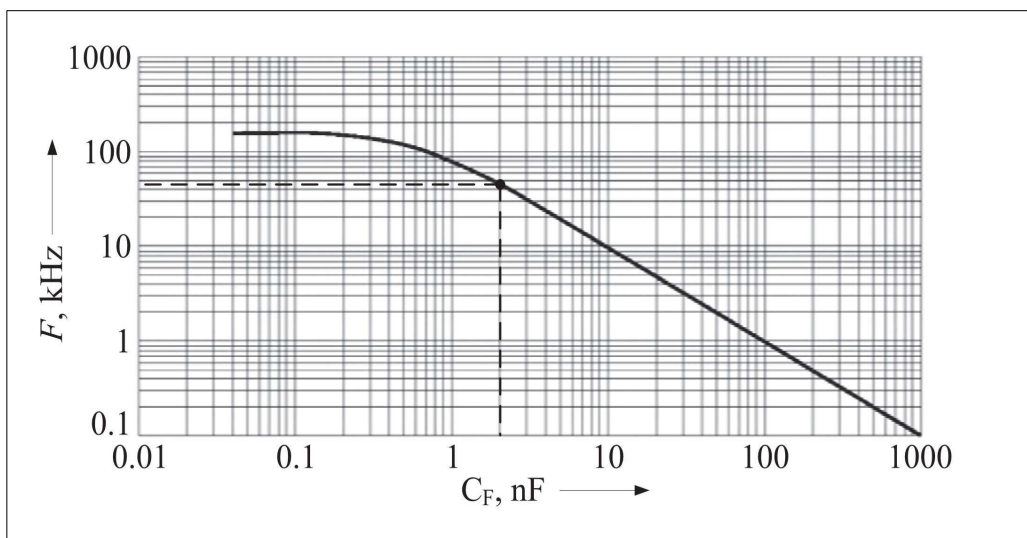


Figure 3. Dependence of the frequency of operation on the value of the $F=f(CF)$

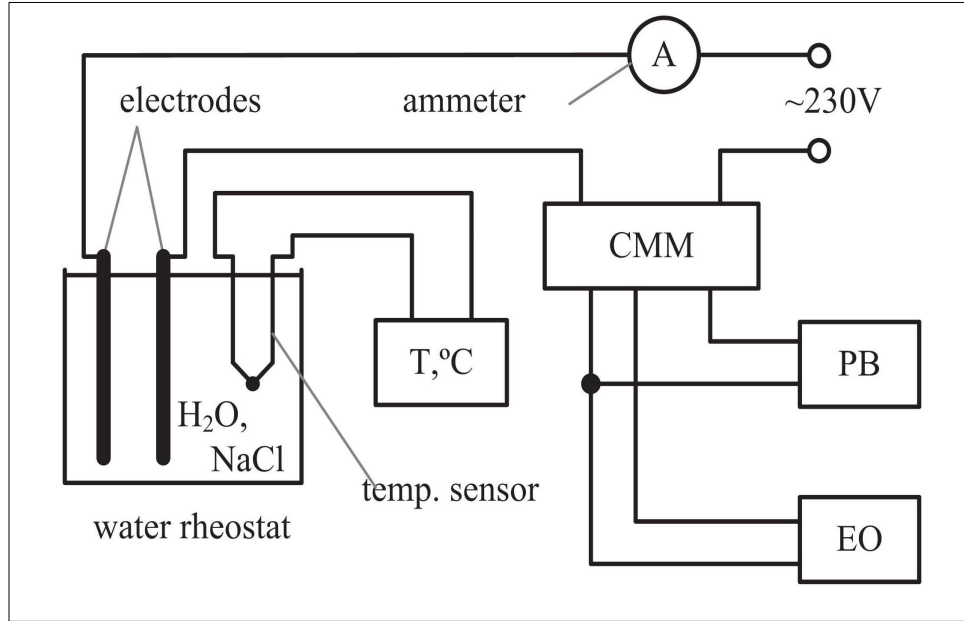


Figure 4. Schematic diagram of the experimental setup

Figure 3 shows the dependence $F = f(C_F)$. It can clearly be seen that at higher capacitance values the operating frequency sharply decreases. Another application of C_F is to adjust the noise steadiness. The low noise steadiness is observed by low capacitance value. So it is necessary when a sensor is used in an apparatus to take into account these two parameters – noise steadiness and speed of work [2]. Figure 3 shows an exemplary selection of the capacitor value C_F limiting the transmit frequency to 45 kHz. This is necessary for further development.

The output of the MIC is at terminal 12 (U_{IOUT}). Its voltage changes in proportion to the magnitude of the measured current I_{TEST}

The schematic diagram of the experimental setup is shown in figure 4.

A water rheostat with NaCl water solution has been used for carrying out the experimental tests. So it is possible to control fuel the current I_{TEST} through measuring module and contactless ammeter.

For the purpose of collecting data for further studies the temperature of the magnetosensitive integrated circuit package T_p and that of the water rheostat T_w solution are also measured. Output data are measured by a two channel electronic oscilloscope (EO).

The obtained experimental transmission characteristics are shown in Figure 5.

They reflect the variation of the output voltage U_{IOUT} from the set current I_{TEST} passing through the sensor module. The analysis of the results shows that the transmission characteristic is linear across the current range ($I_{TEST} = 0 \div 20A$).

From the obtained results the absolute sensitivity SA of the developed device is determined. It is given by the following formula:

$$S_A = \frac{\Delta U_{IOUT}}{\Delta I_{TEST}} \quad (1)$$

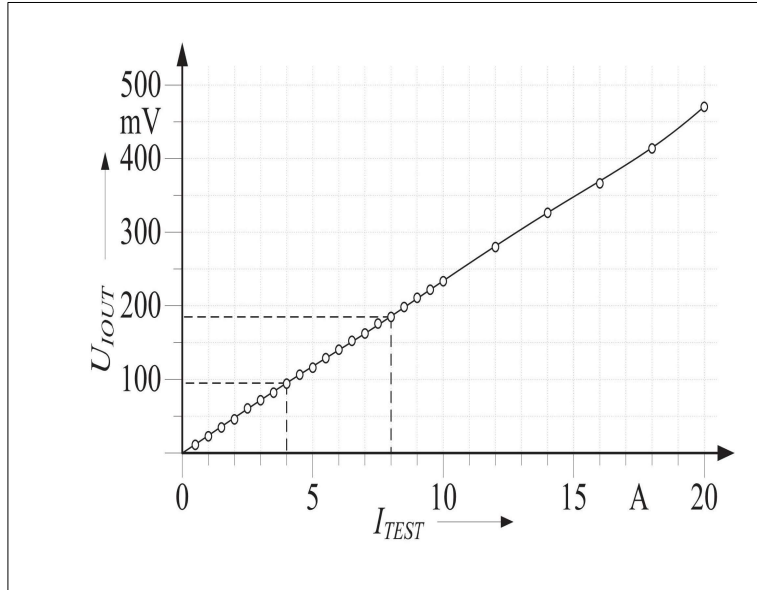


Figure 5. Experimental transmission characteristic $U_{IOUT} = f(I_{TEST})$

where: ΔU_{IOUT} – change of the output voltage from the magnetosensitive integrated circuit; ΔI_{TEST} – the change of the set current, or:

$$S_A = \frac{90,7}{4} = 22,66 \text{ mV / A} \quad (2)$$

From the calculations for the SA it is found that the absolute sensitivity of the test module was kept constant $SA = 22,66 \text{ mV/A}$. For additional information which can help the used module modeling are obtained the characteristics $T_W = f(I_{TEST})$ and $T_P = f(I_{TEST})$. They reflect respectively the water temperature of the water rheostat and that of the magnetosensitive integrated circuit package. The temperature of the chip has a minimal change over the entire operating range, due to the very low resistance of the built-in low resistive copper conductor. The dependencies are presented in the general graph of Figure 6.

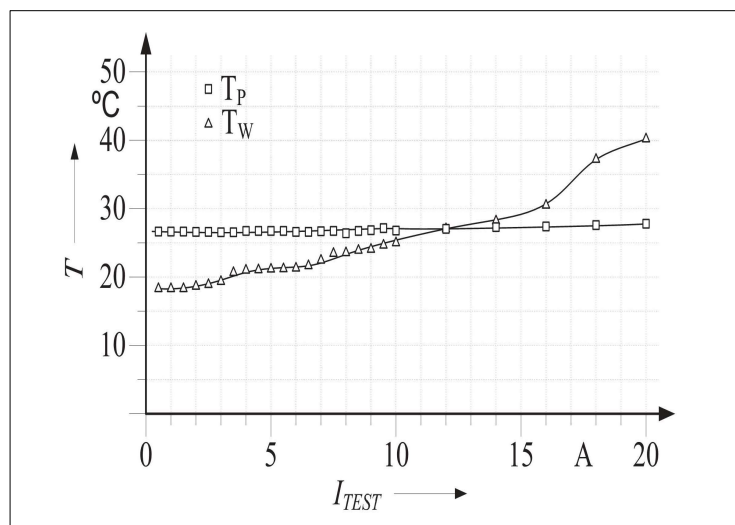


Figure 6. Graphic dependencies $T_P = f(I_{TEST})$ and $T_W = f(I_{TEST})$

The module possibility of feedback realizing when maximum current is reached through external pins of integrated circuit. Low self-consumption power consumption of the module ($I_S < 50\text{mA}$), both in measurement mode and standby mode, and the small dimensions allow him to be built integrated in various electronic devices where it is necessary to measure and monitor the magnitude of the electrical current.

The capability of the conversion feature of the module enables the output electrical signal to be directly coupled to the ADC input thereby simplifying its processing. It is determined absolute sensitivity. It is $S_A = 22, 66\text{mV/A}$.

An experimental set-up was realized (Figure 4). The water rheostat configuration allows the measurement of the electrical current flowing through the sensor to be readily measured. Experimental studies have been carried out and have been reflect the measuring module work.

Transformation characteristics $U_{IOUT} = f(I_{TEST})$ and these reflecting temperature regimes during operation $T_P = f(I_{TEST})$, $T_W = f(I_{TEST})$ at different values of the measured current $I_{TEST} = 0, 1 \div 20\text{A}$ are built in sequence.

Developed and tested device is intended for installation in a variety of instrumentation and devices allowing its output signal to be used to measure and build feedbacks monitoring of various electrical parameters of the power circuits.

References

- [1] Draganov, N. (2014). Contact-Less Galvanomagnetic Ammeter for AC and DC. *Journal of Mechanical engineering and electronics*, Vol. 3. ISSN: Sofia, p 0025–455X, Crp.40-43.
- [2] Draganov, N. & SENSORS Principle, structure, technologies, characteristics, parameters and applications, *Vol. 1. Publishing House X-Press Gabrovo*. Bulgaria (2014).
- [3] Draganov, N. Galvanomagnetic contractless protection of AC induction motor. *Journal of the Technical University of Gabrovo*, Vol. 46. Gabrovo, Bulgaria (2013), ISSN 1310-6686, p 84–88.
- [4] Draganov, N.D. (2014) Experimental digital three-phase check electrical energy meter. Part 1. *Proceedings of the Papers of International Scientific Conference ICEST*, Vols. 25–27. Juny: Niš, Serbia, ISBN 978-86-6125-109-2, p 429–432.
- [5] Draganov, N. & Draganova, T. Based of AMR sensors device for Multicannal contractless measurement of AC current. *Journal of the Technical University of Gabrovo*, Vol. 41. Gabrovo, Bulgaria (2011), ISSN 1310-6686, p 84–87.
- [6] Penchev, P. (2014). *Measuring in Electronics*. Vasil Aprilov Print. Gabrovo, Bulgaria.
- [7] Lozanova, S., Altunyan, L., Noykov, S., Ivanov, A. & Roumenin, C. (2017), 17-18 Nov. 2017 Temperature influence of Hall sensor nonlinearity. *International Scientific Conference UNIV. TECHNOL.* Gabrovo, Bulgaria, p 341–345.
- [8] Roumeni, C. (1994) *Solid state magnetic sensors (handbook of sensors and actuators)*. Elsevier, 2.
- [9] Allegro Microsystems. www.allegromicro.com data sheet of sensors 20.11.2018.
- [10] Digikey, www.digikey.com/en/articles/techzone/2012/sep/thebasics-of-current-sensors